THX
CERTIFIED PROFESSIONAL
VIDEO CALIBRATION

CalMAN Studio

Naples Display Calibration

Buzz Schranz
Email: buzz@naplesdisplaycalibration.com
Phone 1: 1 239 248 5069

METER Klein Instruments K Series

Manufacturer: Klein Instruments
Model: K-10
Meter Serial: 00100001

SOURCE AccuPel DVG-5000

Model: AccuPel - DVG-5000 (RS-232 @9600, USB)
Info: DVG-5000 v4.73 COM4

IMAGE PROCESSOR ColorBox 3D Cube Processor

Model: SpectraCal - ColorBox (USB)
Type:
Info1:

CALIBRATION STANDARD

Input Signal Levels	NominalLevels: True
Luminance Response Target	GammaFormula: PcGamma: 2.2
Color Gamut Target	Gamma:

SpectraCal

Naples Display Calibration

Contact Name: Buzz Schranz
Phone 1: 1 239 248 5069 Email: buzz@naplesdisplaycali

PRE-CHARACTERIZATION OF DISPLAY

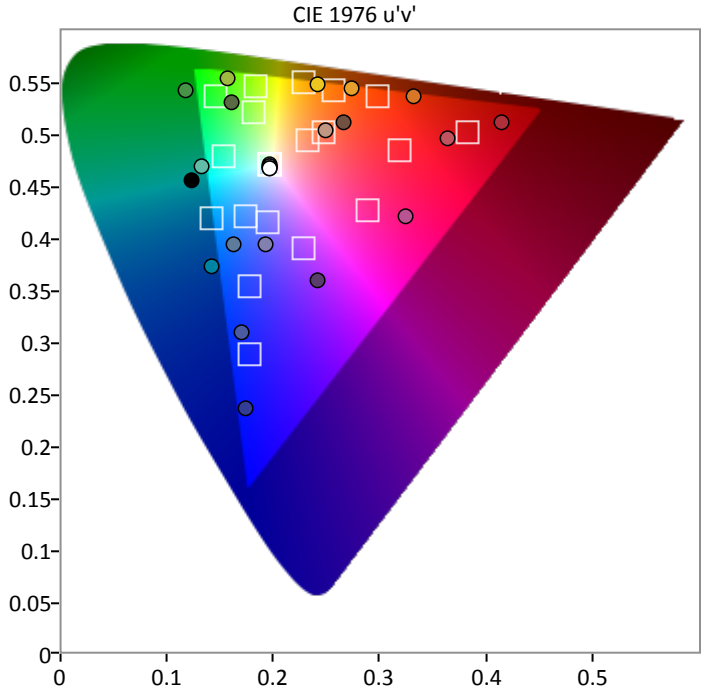

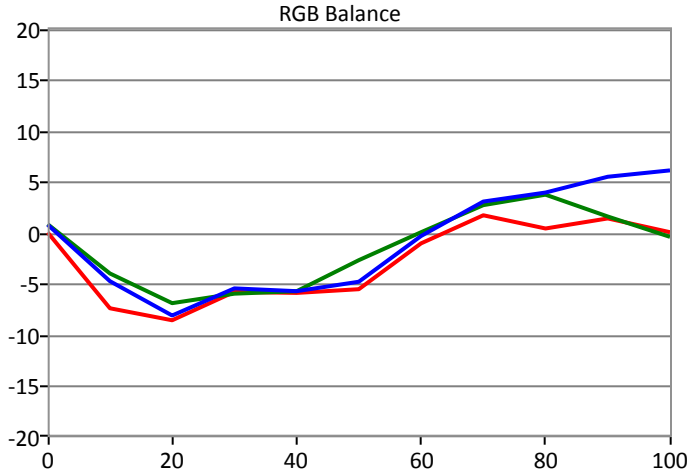

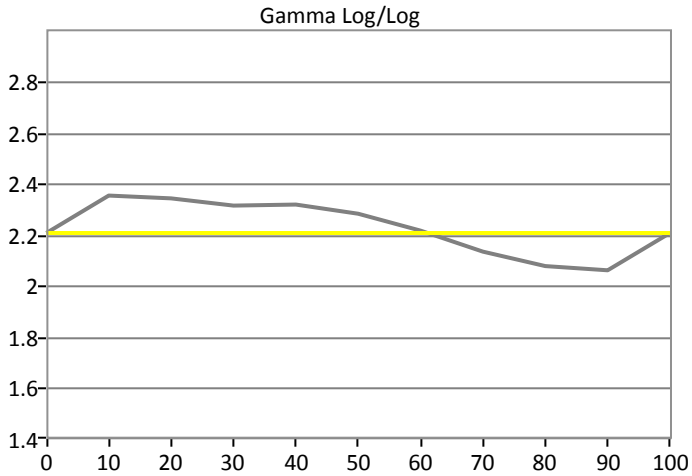

POST-CHARACTERIZATION OF DISPLAY

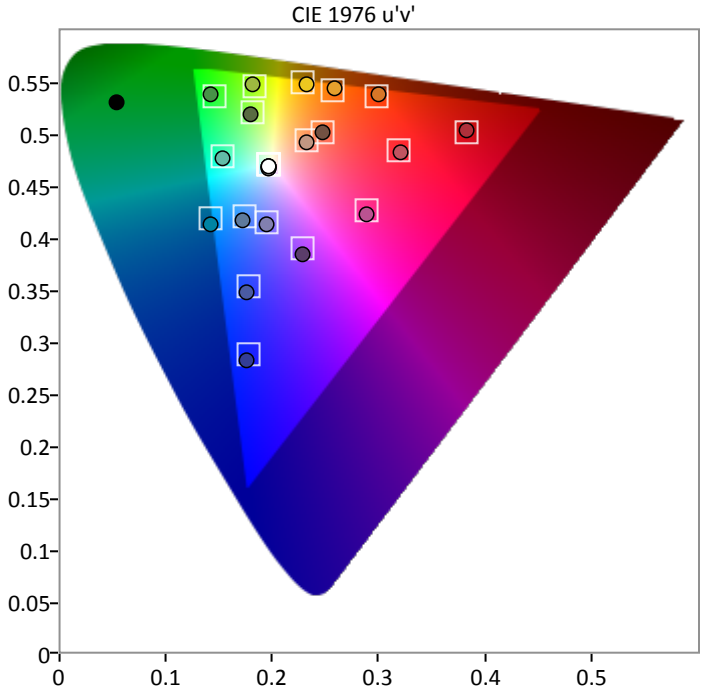

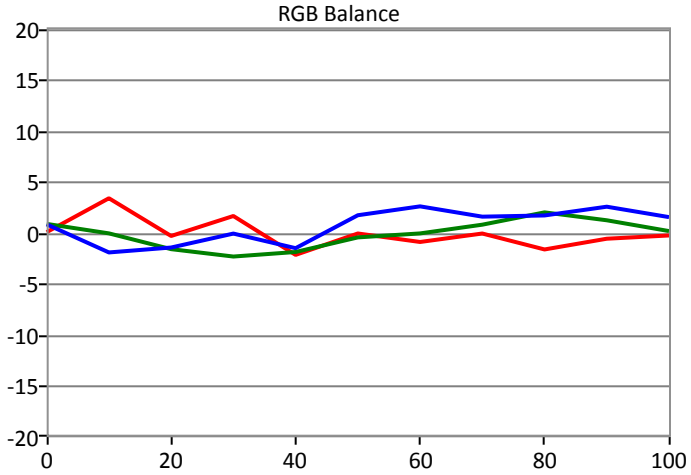

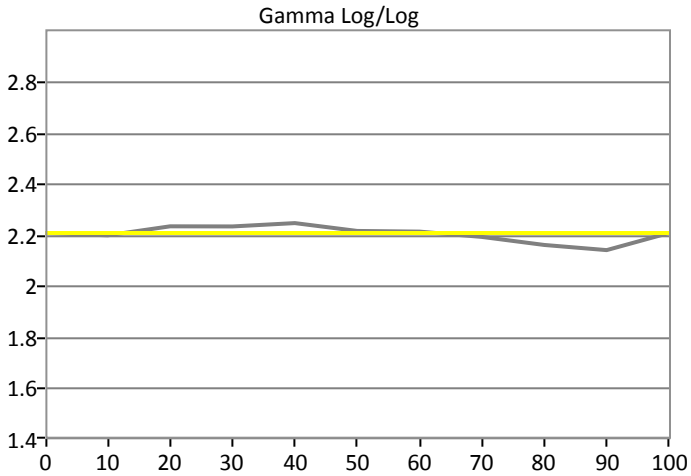

Naples Display Calibration

Contact Name: Buzz Schranz
Phone 1: 1 239 248 5069 Email: buzz@naplesdisplaycali

PRE AND POST-CHARACTERIZATION OF DISPLAY

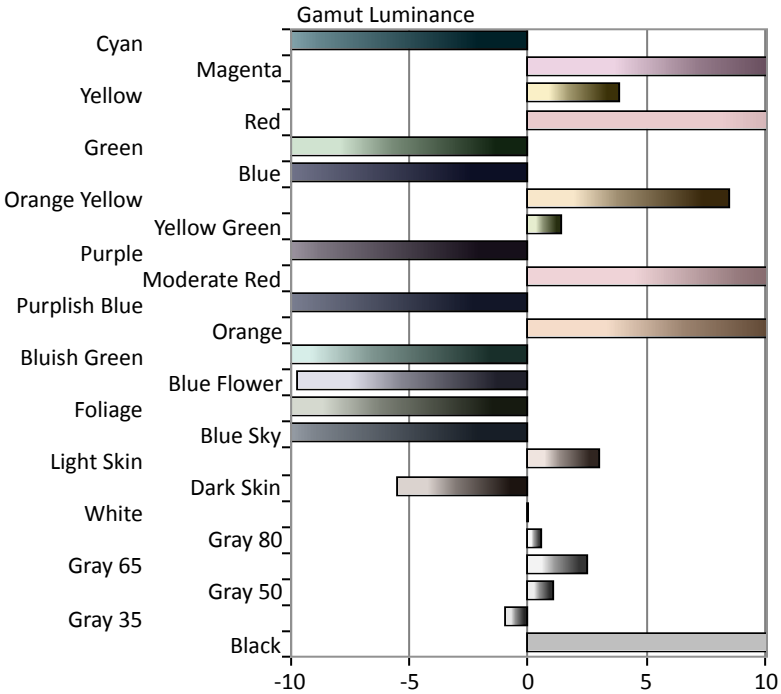

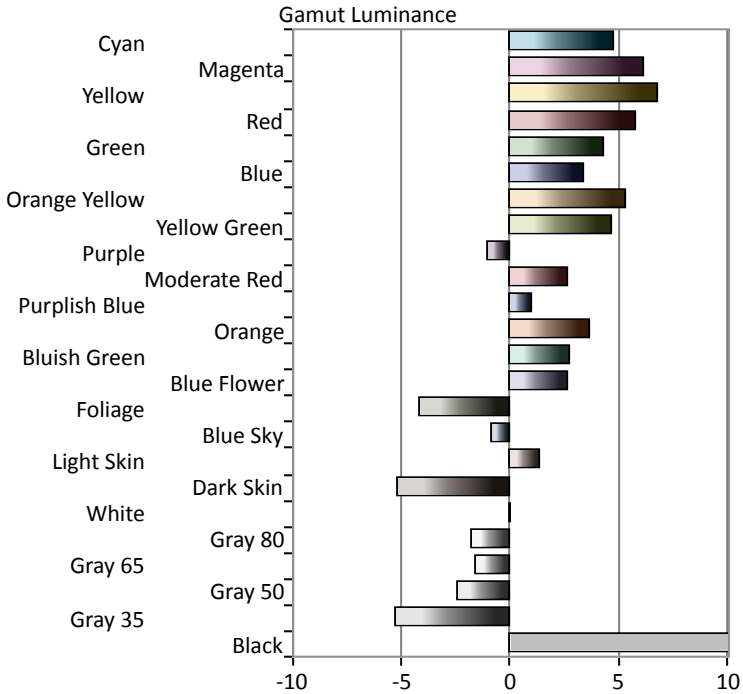

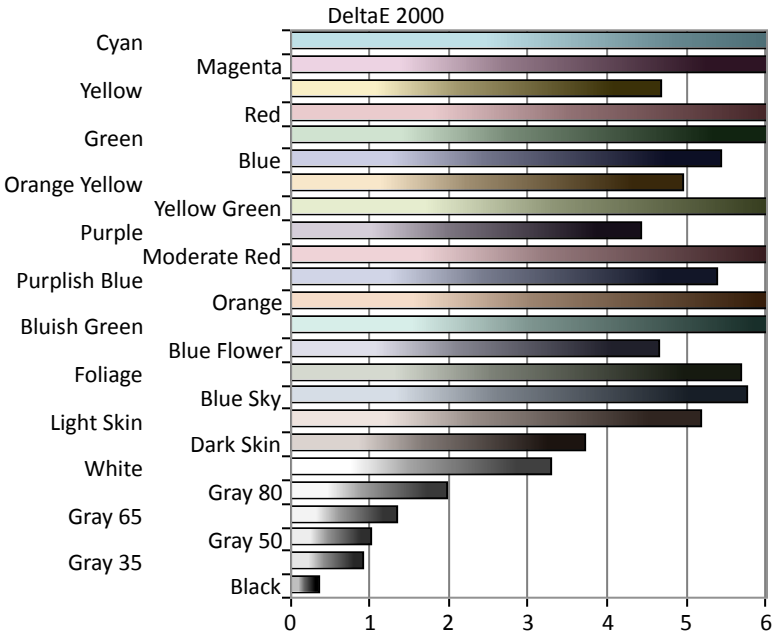

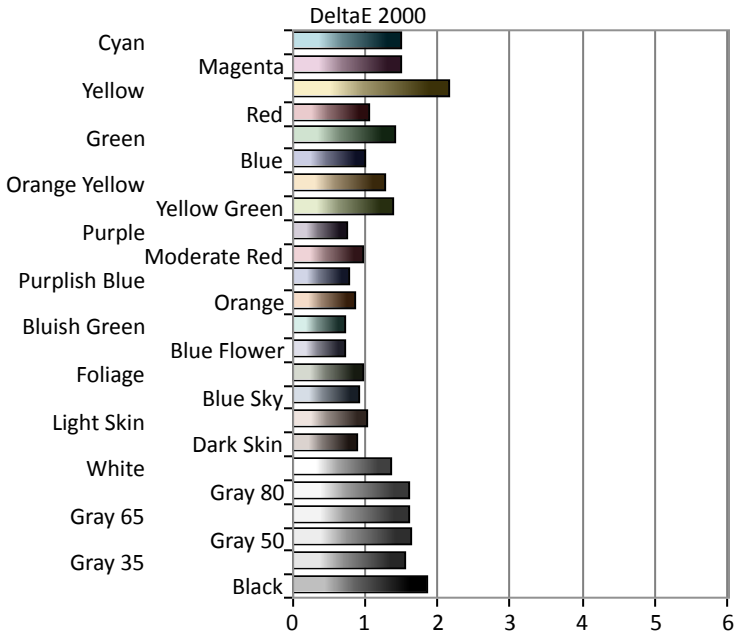

3D LUT CUBE DATA RESULTS

Cube Points: 0 Points

White Point dE: 0.7

Contrast Ratio (ON OFF): 5198

Average dE: 0.5

Y Max: 49.78 fL

Max dE: 2.6